



# Allergan 3-laser, 8-color (4-2-2)

Cytometer:	FACSCantoII	User:	Administrator
Cytometer Name:	FACSCantoII	Institution:	N/A
Serial Number:	V33896202019	Software:	BD FACSDiva 8.0
Input Device:	Manual	Date:	1/20/2015 10:02:03 AM
Window Extension:	7.00		


Blue Laser  
(488nm)  
FSC

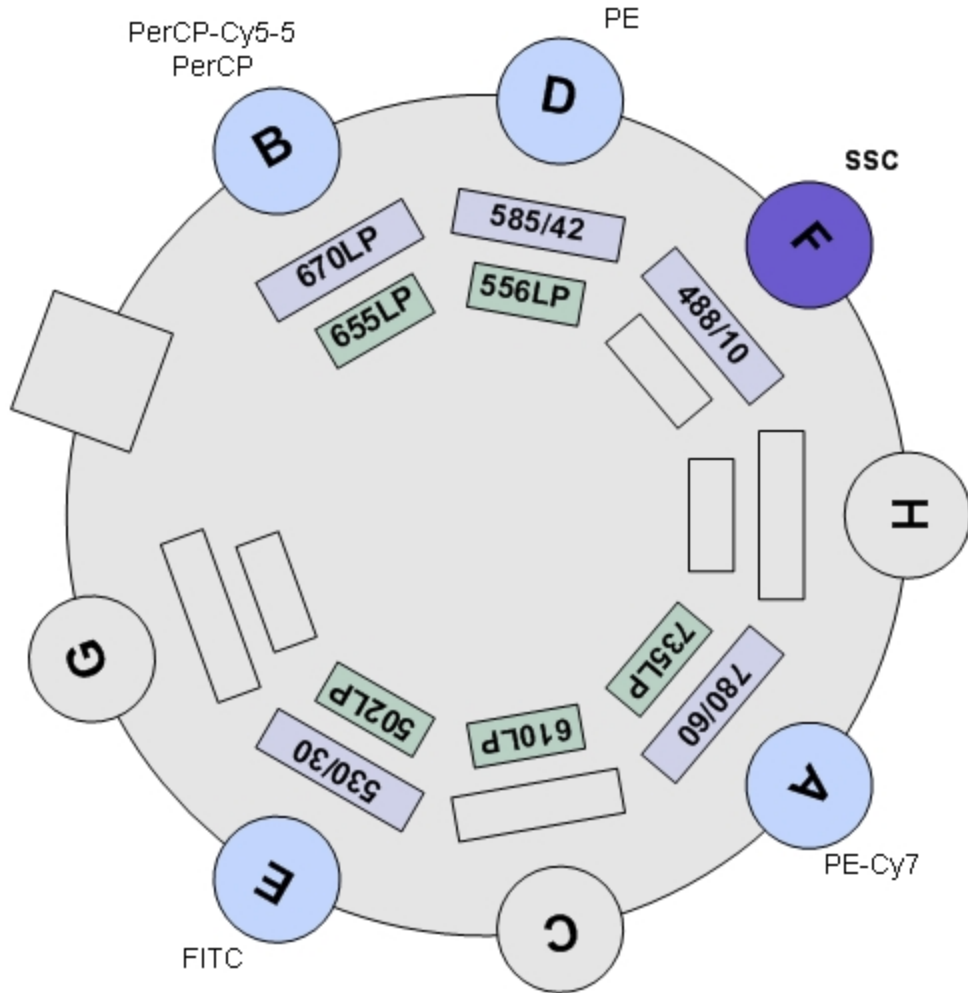

Red Laser  
(633nm)

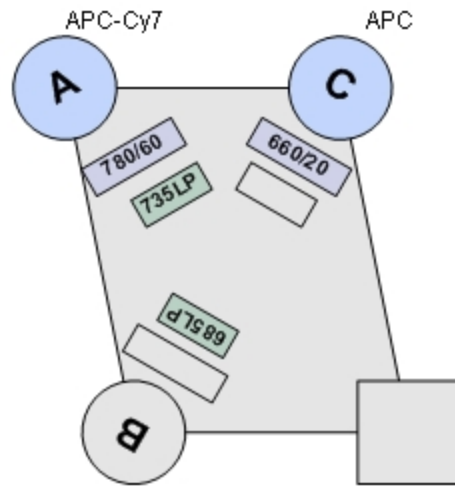

Violet Laser  
(405nm)

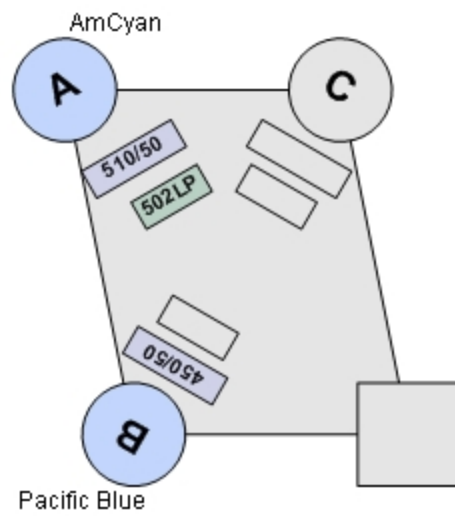

Comments: