



Cantoll YellowGreen Carousel

Cytometer:	FACSCantoll	User:	Administrator
Cytometer Name:	FACSCantoll	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0
Input Device:	Manual	Date:	9/28/2017 2:15:56 PM
Window Extension:	7.00		


Red Laser (633nm)

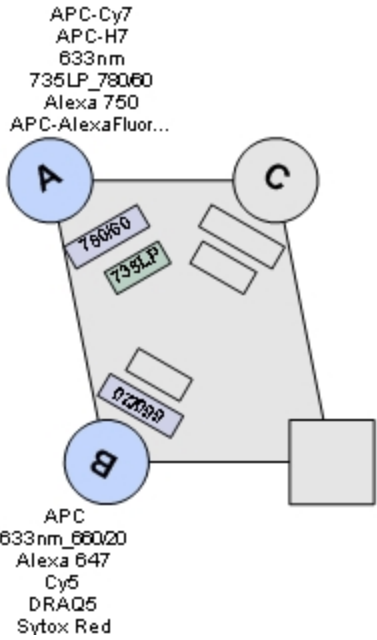

Blue Laser (488nm) FSC

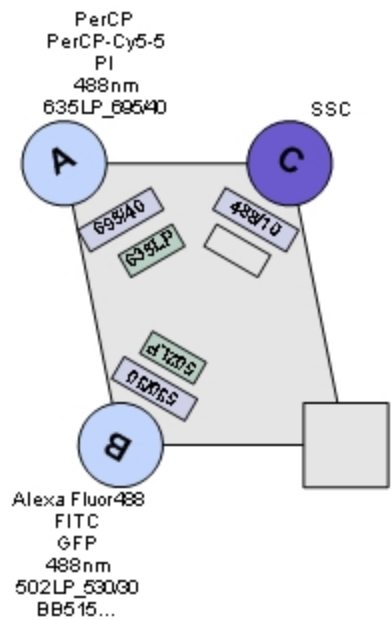

Yellow-Green Laser

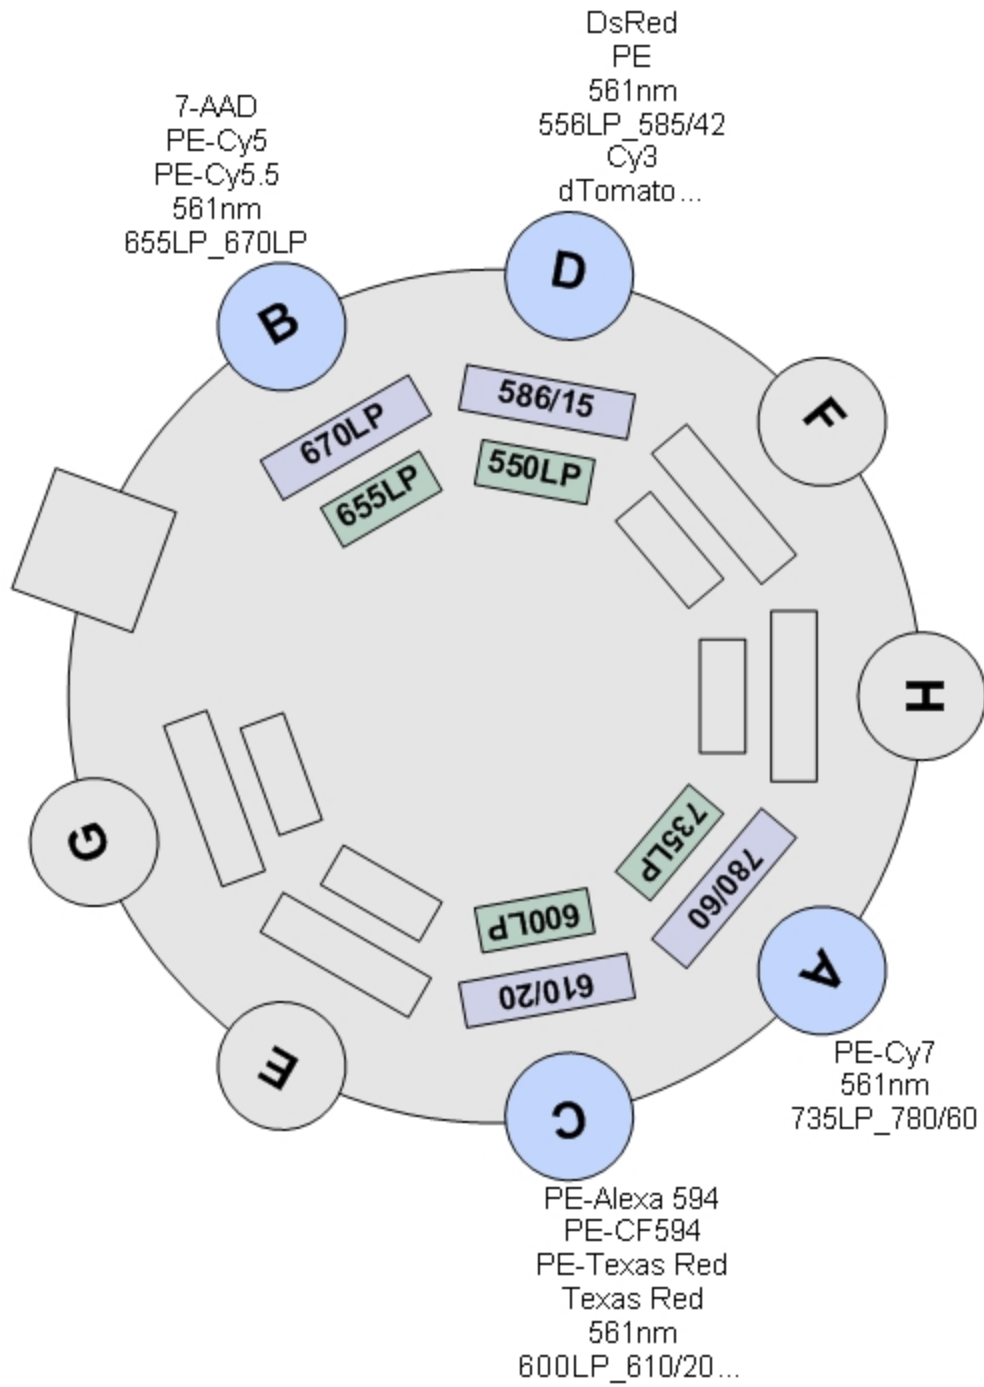

Comments: