



# 100um BCM-THI 2B-3R-6V-4YG-3UV

Cytometer:	FACSAriaIII	User:	Administrator
Cytometer Name:	FACSAriaIII	Institution:	N/A
Serial Number:	R65828200106	Software:	BD FACSDiva 8.0.3
Input Device:	Manual	Date:	4/16/2026 3:11:22 PM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	2.00		


Blue Laser  
(488nm)  
FSC

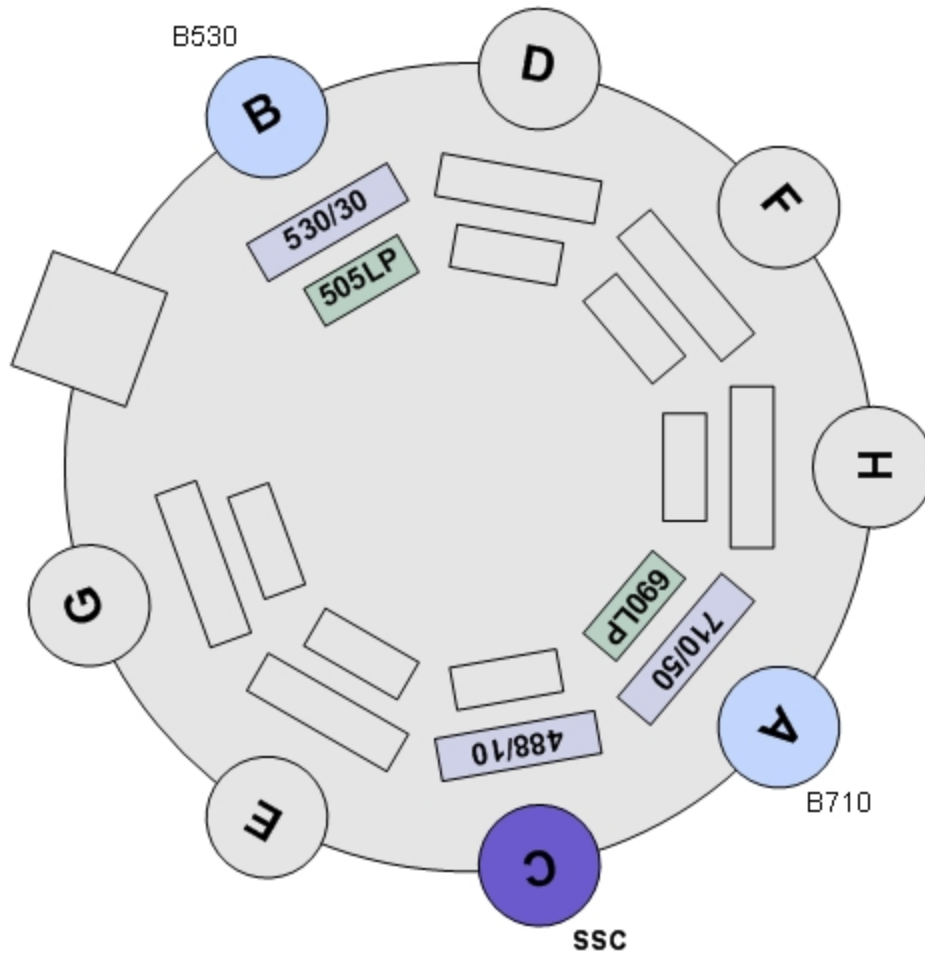


Violet Laser  
(405nm)

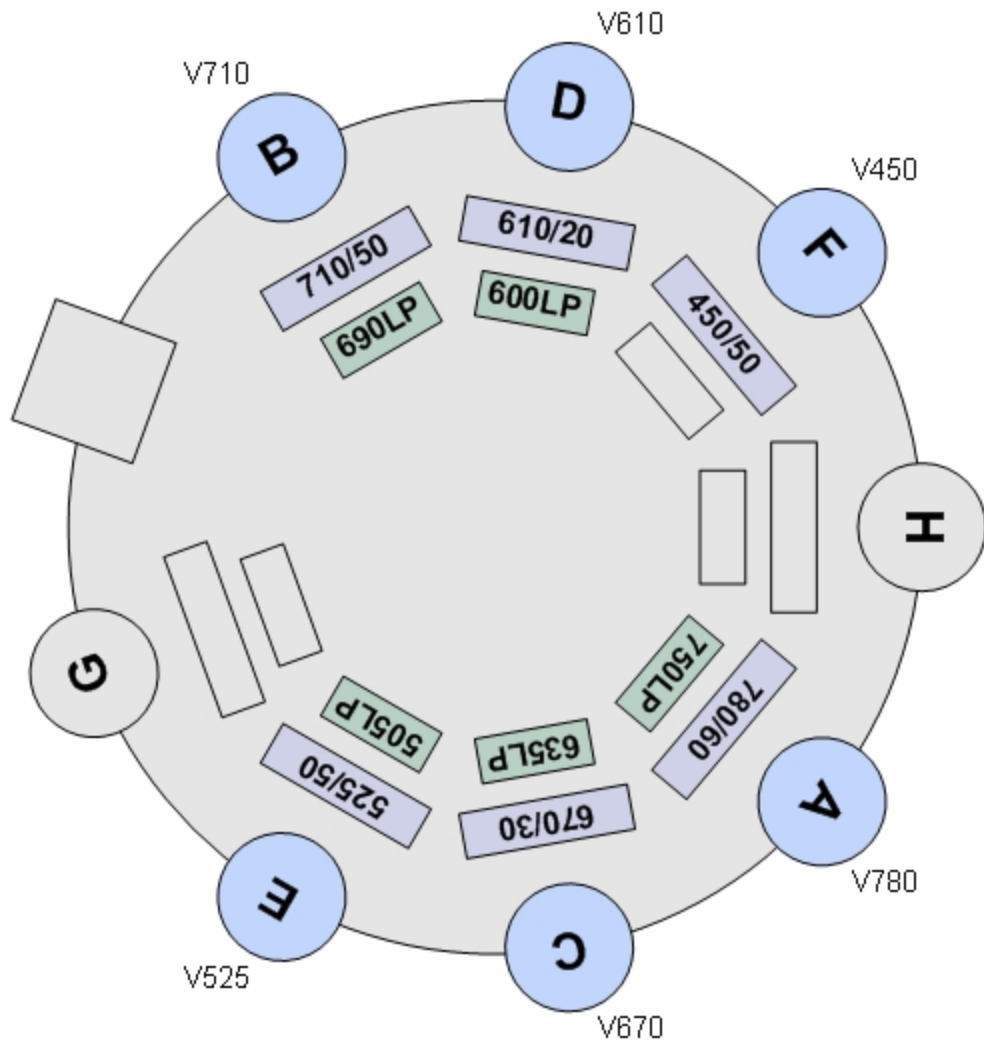


YG Laser  
(561nm)

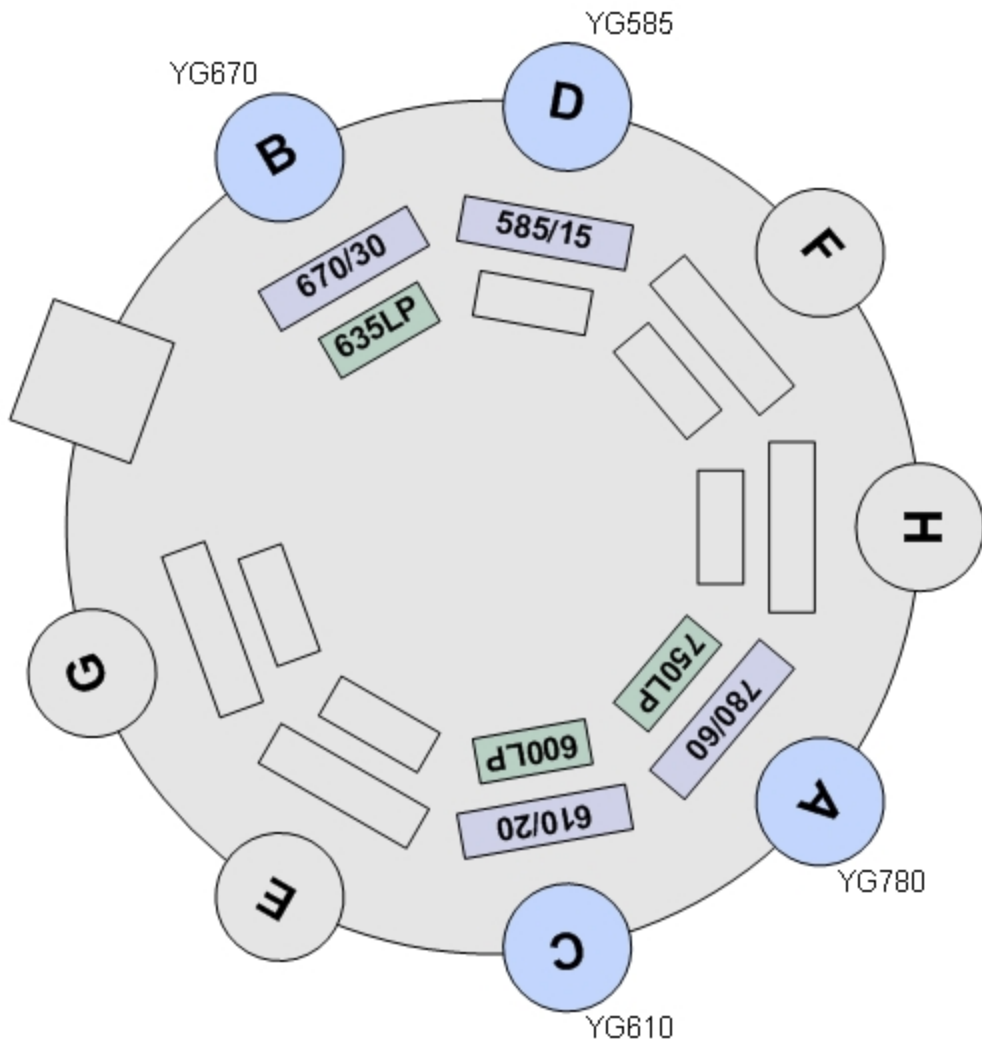

Red Laser  
(637nm)

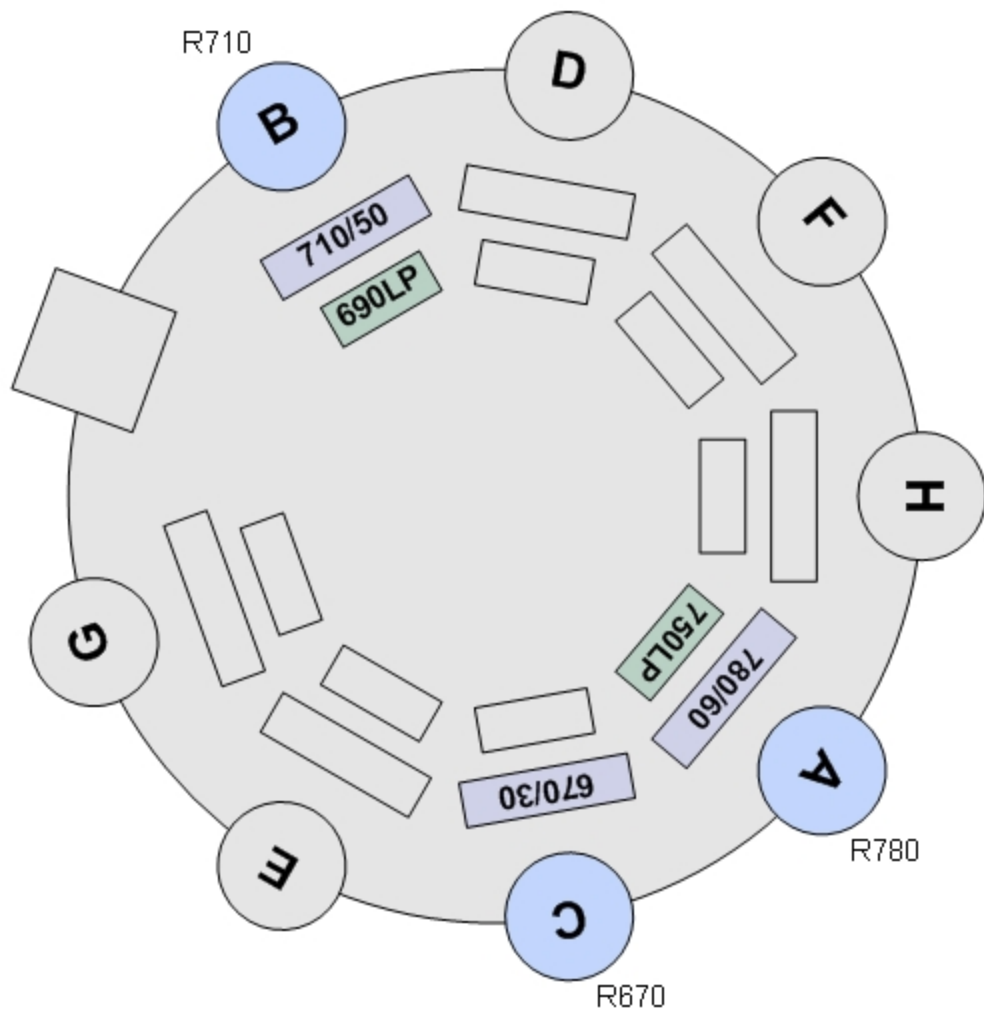

UV Laser  
(355nm)

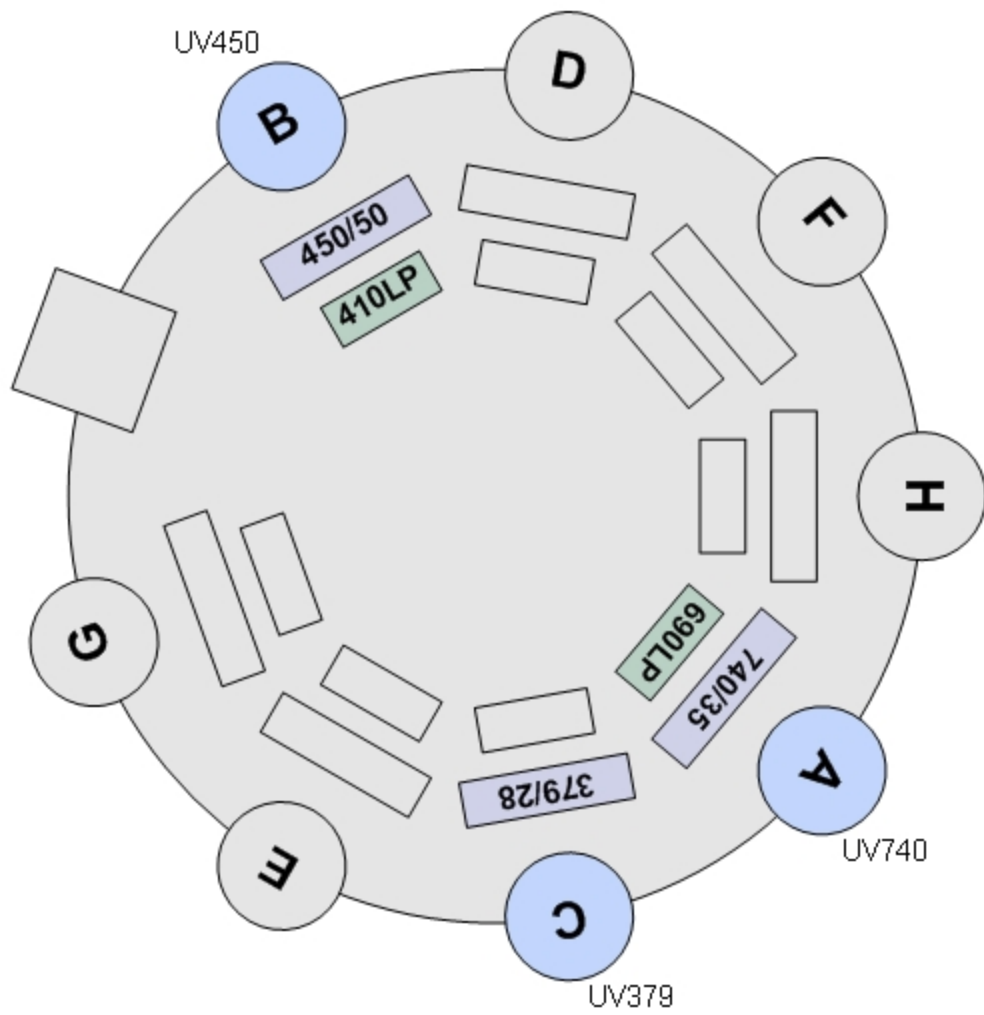

Comments: