



190909 Fortessa T103 V.2

Cytometer:	LSRII	User:	Administrator
Cytometer Name:	LSRII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 9.0
Input Device:	Manual	Date:	5/11/2026 7:47:28 AM
Window Extension:	10.00		


Blue Laser
(488nm)
FSC

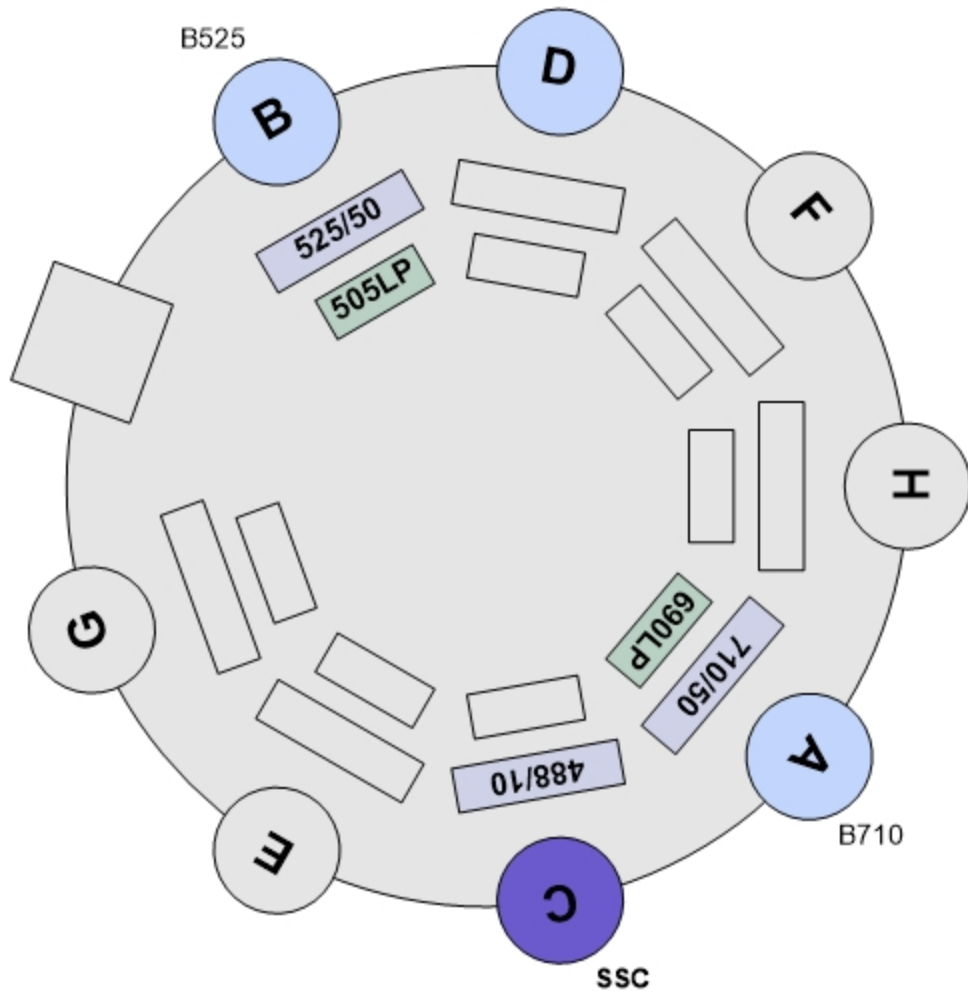


Violet Laser
(405nm)

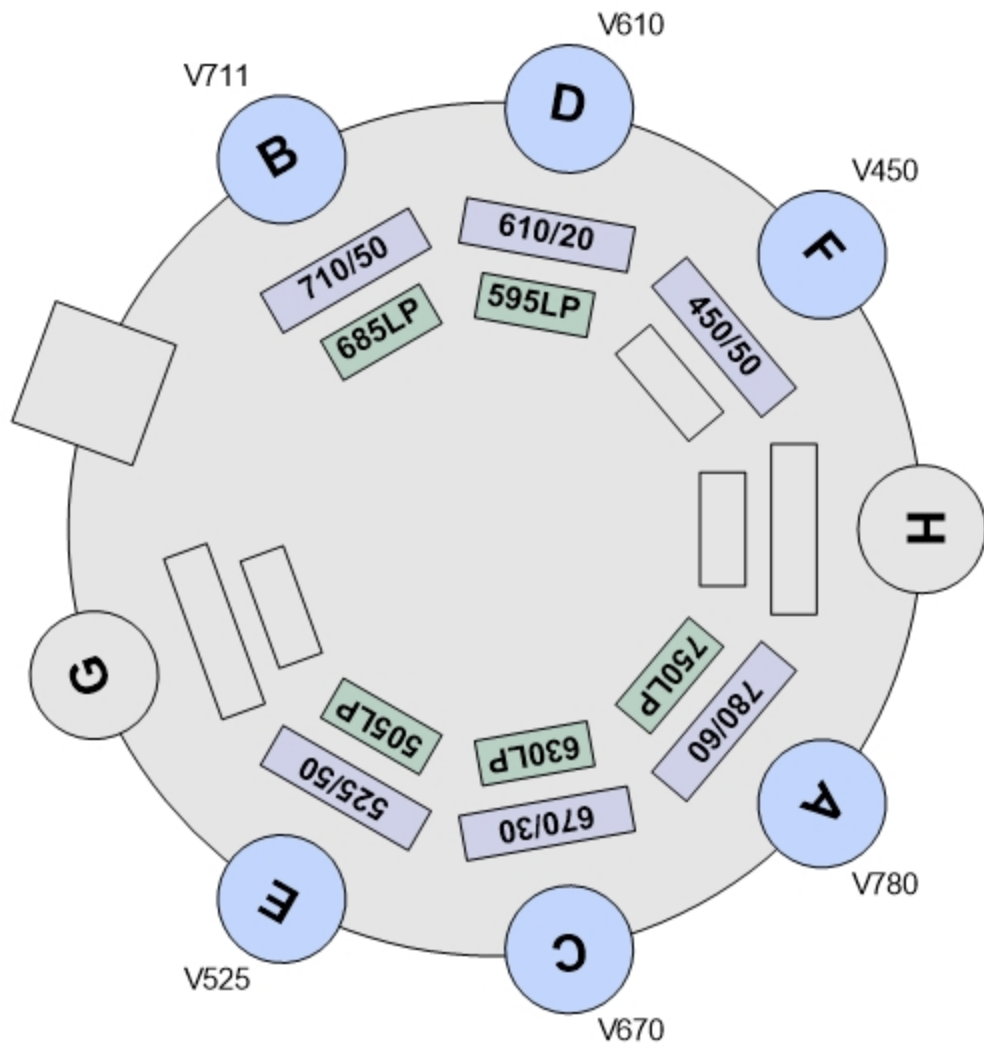


Red Laser
(640nm)

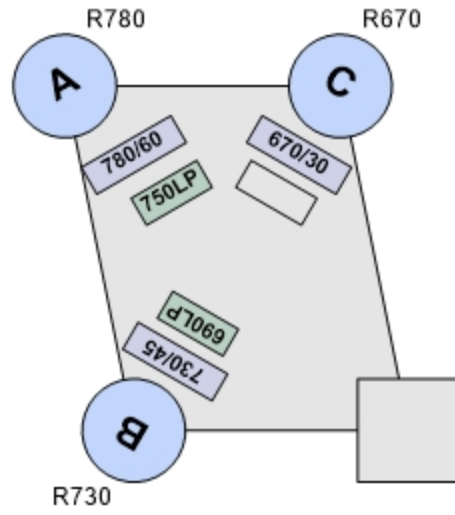

UV Laser
(355nm)

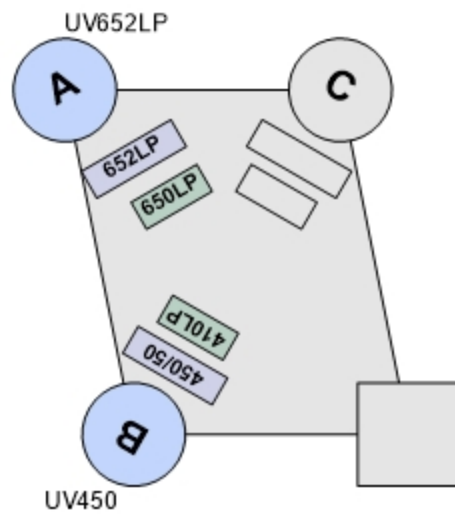

YellowGreen Laser
(561nm)

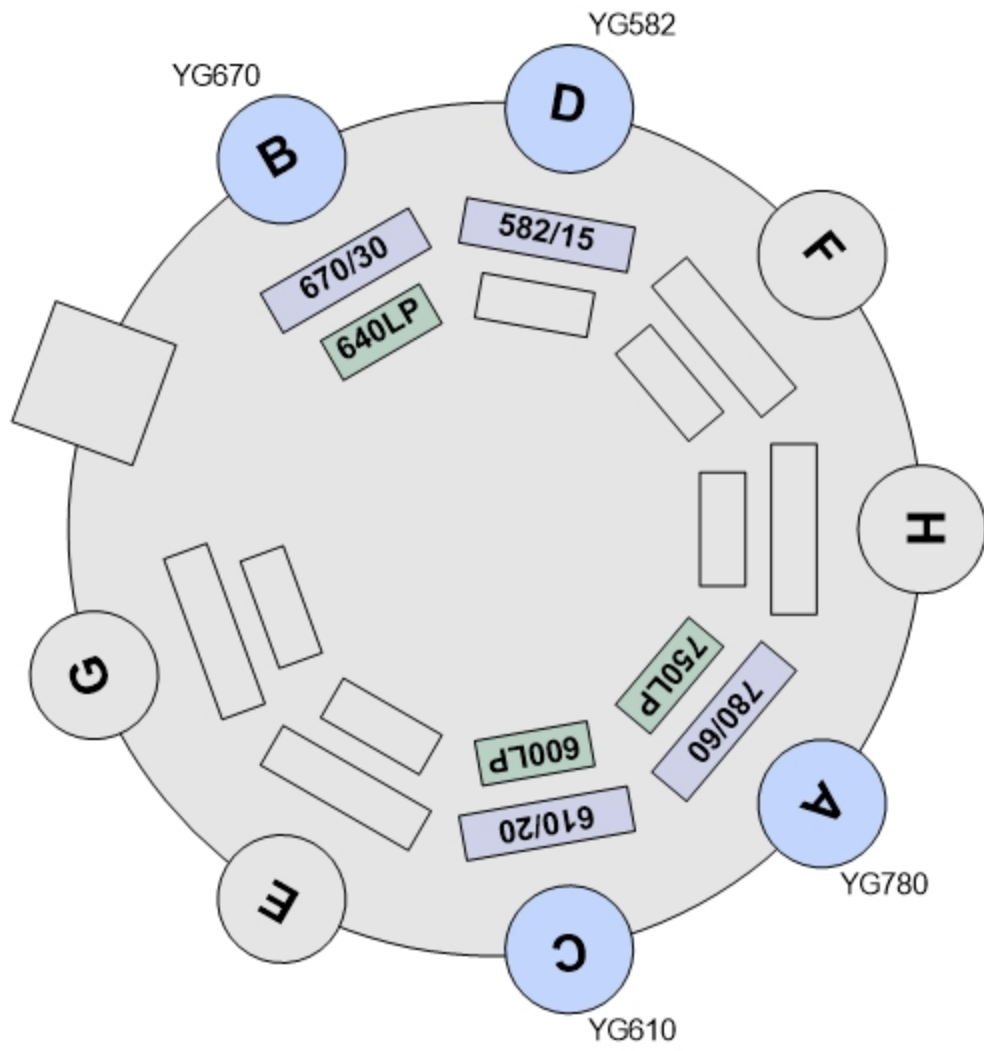

Comments: